



Audio Engineering Society Conference Paper

Presented at the International Conference on
Acoustics & Sound Reinforcement
2024 January 22–26, Le Mans, France

This paper was peer-reviewed as a complete manuscript for presentation at this conference. This paper is available in the AES E-Library (<http://www.aes.org/e-lib>), all rights reserved. Reproduction of this paper, or any portion thereof, is not permitted without direct permission from the Journal of the Audio Engineering Society.

Comparative Evaluation of Public Address Feedback Controllers: A Preliminary Assessment Methodology

This Conference uses blind reviewing, do not put author names, leave this space blank. On acceptance you will receive a new template to add author information.

ABSTRACT

Anti howling (AH) systems a.k.a. acoustic feedback control allow to maintain sound quality and prevent the howling effect in public address (PA) systems. Various principles may be used for AH, each with its advantages and drawbacks. The objective of the present work is to propose a methodology for evaluating commercial or simulated AH systems as "black boxes". Following previous publications, the evaluation is based on three critical aspects : the Additional Stable Gain (ASG) which is achievable before Larsen howling occurs, the Perceptual Evaluation of Speech Quality (PESQ), a standardized speech quality criteria, and the "Reactivity" which quantifies how fast the AH device adapt to changes of the electroacoustical environment. Preliminary results are presented for six different AH systems. They illustrate that the proposed protocol allow to distinguish small differences between designs, in addition to highlight the general trends already described in the existing literature.

1 Introduction

Many audio applications include situations where a microphone may sense the acoustic pressure radiated by a nearby loudspeaker, leading to potential drawbacks. Classical examples include the local echo within a hand-free telephone set [1], audio feedback within a hearing aid [2] or acoustic feedback within a PA system used in live amplification, potentially leading to the well-known Larsen effect or "howling" [3]. Although some musical styles include the intentional use of feedback, especially for electric guitars, most situation require to prevent howling. This is primarily done using carefully placed directive microphones and speakers and adequate tuning of the PA system. This allows to cope

with various situation, excepting venues with a poor acoustic behaviour [4].

Indeed, the influence of the room over sound transmission has been studied for a long time [5], including its effect on PA systems stability [6]. Room response may be considered as a random process, although for given locations of speaker and microphone, at given environmental conditions, it may be considered as a linear system combining many acoustic paths and thus leading to a very irregular frequency response showing dips and peaks. This frequency response is combined with the one of microphone, speaker and processing equipment, building a closed-loop system which must obey classical stability criteria in order to avoid howl-

ing [7]. However, the characteristics of the acoustic paths within a room change with time and this requires to tune the PA system accordingly in order to keep its stability. Numerous solutions have been proposed to cope with automatic tuning of a PA system in order to avoid howling, and eventually to increase its stable gain without degrading much the amplified signal quality. Such systems are globally called "Anti-Howling" (AH) systems in this paper. A comprehensive and well-argued review has been proposed by Van Waterschoot and Moonen [8], who proposed to distinguish four classes of AH methods: time-varying filters, gain reduction methods, spatial filtering methods, and room modeling methods.

These methods are implemented in various systems, each possessing distinct features and being more or less effective depending on given practical situations. It is thus difficult to rank them objectively using a single criterion: many papers have proposed comparisons within a given class of AH method but few of them tried to give an overall assessment method allowing the comparison of a wide range of AH systems. This is the objective of the present work, which proposes a combination of previous assessment methods and its implementation using affordable tools. Section 2 give a short description of the main AH methods proposed in the literature, allowing to understand their specificities. Their comparison is based on previous work about AH systems evaluation, presented in section 3. The proposed assessment method is then described by section 4 and first results are shown in section 5

2 Main anti-howling (AH) methods

Figure 1 outlines the single path (SISO) structure considered here for a sound reinforcement chain : the linear electroacoustic path $[F]$, some potentially non-linear processing $[G]$ and the anti-howling system $[H]$. Multi-input or multi-output (MIMO) configurations are not considered in this preliminary work.

Basic principles of AH system are summarized below, following the classification already proposed [8] but excluding the MIMO spatial filtering methods.

2.1 Time-varying filters

In order to avoid a stable in-phase condition for the feedback path, several principles have been proposed

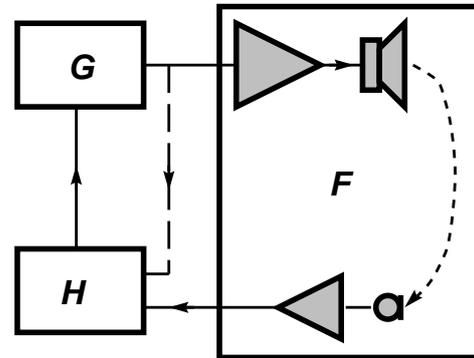


Fig. 1: Diagram of a sound reinforcement chain containing an anti-feedback system $[H]$, a processing module $[G]$ and an electroacoustic path $[F]$.

: the earlier is frequency shifting (FS) [9]. Other time-varying filters such as phase (PM) or delay (DM) modulation have also been considered. Their drawback is a sound modulation which may be acceptable for speech but less for music [10]. A small amount of PM is however interesting as a mean to improve other AH methods [11].

2.2 Gain reduction

The most straightforward AH method is to mimic a sound engineer: reducing the system gain, either globally (AGC) [12], or by automatic equalization of critical frequency bands (AEQ) [13]. An alternative, widely used in commercial systems, is the so-called "Notch-filter-based Howling Suppression" (NHS) [14] which detects howling and activates notch filters tuned to the instability frequencies.

2.3 Room modeling

A very efficient AH method is based on a model of the electroacoustic loop (the $[F]$ block in figure 1). This model may be used to equalize the overall response or to subtract the loudspeaker contribution from the microphone signal, a technique we call "Acoustic Feedback Removal" (AFR) as the AFC acronym is ambiguous. Compared to the acoustic echo cancellation (AEC) used in telecommunication, AFR has to cope with a high correlation between the wanted and unwanted signals, thus requiring a decorrelation mechanism. Many techniques have been proposed for this purpose, leading

to various algorithms [8, 15, 16, 17, 18]. While AFR may be CPU-demanding, it has no theoretical limit to the potential improvement in stable gain.

3 Evaluation of AH systems

The comparison of AH systems require to find evaluation criteria adapted for all the principles described above, and combinations of them. Early work dealt with the investigation of feedback in PA systems, considering how equalization techniques might improve the maximum gain, the audio quality and the robustness of the system [19]; this work did not however consider AH systems yet. Later, as standard about AEC included a few evaluation criteria focused on the echo reduction [20]; it did not take into account some specificities of AH systems.

Later work did target the performances of AH systems : Time-varying AH systems have been compared in a publication, mainly in terms of "gain before instability" (GBI) - in fact its increase [10]. Several publications dealt specifically with AFR systems : Bispo [21] used a virtual environment, using "misalignement" (MIS) criterion to assess the internal filter identified for AFR. Numerous publications dealt with the specific application of AH systems used in hearing aids [22]. The criteria used in these works were different for each class of AH system, and thus did not allow a generic evaluation.

A recent publications proposed a comparison of the performances of several AH system principles, based on two criteria common to all AH systems : the "added stable gain" (ASG also often denoted ΔMSG) and an objective quality criteria : "spectral distortion" (SD) [23]. This publication was followed by a review including a comparison of several AH systems, based on simulations [8]. In addition to MSGI and SD, this paper proposed two criteria about "reliability" : "howling occurrence probability" (HOP) and "time to recover from instability" (TRI).

The howling detection is a subject by its own, as it is both a component of NHS-based AH systems and a tool for the assessment of ASG. Specific evaluations of howling detection criteria have been proposed [24, 25, 26]. The authors compared numerous criteria for howling detection using the Receiver Operating Characteristic (ROC), a statistical plot of the true positive rate against the false positive rate.

3.1 Challenge evaluating a commercial system

Many of the publications about AH evaluation were based on simulations of the various systems to compare. This allows the access to internal quantities (signal, filters, freeze signals, etc) which are not always available in commercial system - especially when AH is an embedded function inside a large piece of equipment, like an audio mixer. Some authors proposed an implementation using a DSP board to speed up AH systems comparison [27]. The AH systems were however only AFR-based and implemented as computer codes.

To compare "black-box" commercial systems, the only way is to design a protocol using only their input and output, with suitable test signals. Such a protocol was proposed by some authors in order to evaluate commercial hearing aids [28]. A fair comparison is however difficult : the authors mentioned that measurements of the ASG for four different input signals showed that ASG depends on the input signal. Moreover minor changes in the set-up may cause significant feedback path differences at higher frequencies.

Using physical setups has thus the drawback that it does not allow independant comparisons by different actors, even using standardized facilities. We therefore propose to use a virtual acoustic environment (with characteristics representative of a "typical" PA situation), which could allow to get comparable results between measurements performed in different locations or at large time intervals.

3.2 Evaluation criteria

Three criteria, selected from both existing literature and common audio practices, have been chosen because they directly address the most critical aspects of an AH system's performance.

3.2.1 Added stable gain

An important criterion for evaluating AH system is the gain (ASG) which can be added to the system when the AH system is used, compared to when it is not used. Even if this criterion is less important for PA system than for hearing aids, it is still a major one. With no access to any internal quantity, this criterion must be based on a general gain estimation.

In most experimental publications [8], ASG is determined by incrementally raising the gain of the direct

path $[G]$ until instability occurs, both with and without the acoustic feedback controller (AH) active. ASG is then supposed to be the difference in gain between these two conditions, but this is not true if the AH system changes the overall gain of $[H]$, as in NHS systems. Moreover, instability onset is difficult to identify so the estimates often depend on the operator.

A solution is to evaluate the gain as the ratio of averaged Power Density Functions (PSD) between input and output of $[H]$, estimated with and without AH. A further correction of the instability onset estimation may be performed when both $[G]$ and $[F]$ are linear and invariant, as explained in section 4.

3.2.2 Audio quality

Maintaining high audio quality is crucial in any PA system. Early works [8] introduced objective criteria, such as spectral distortion (SD) but did not link them to the listener experience. Some authors [22] then proposed to add objective criteria based on perceived audio quality, such as PESQ for speech or PEAQ for music.

Such objective quality measure for speech and music signals can yield inconsistent results when applied together [29]. As a result, separate measures are required for speech and music evaluations. This paper focus on PA systems mainly for speech reproduction, and thus only consider PESQ which was originally developed by the ITU-T for evaluating speech quality in the context of speech coding for telecommunications.

PESQ has since found utility in assessing the impact of various types of distortions, including acoustic feedback [30]. It compares a reference (original) speech signal to a degraded (processed) version and assigns a score between -0.5 and 4.5, with higher scores indicating better speech quality. In this paper, the reference signal is the one to be reproduced, while the test signal is the one measured as the output of the PA system (including the AH and acoustic feedback).

3.2.3 Reactivity

Previous works [8] also evaluated the robustness of AH systems, using various criteria, among which "time to recover from instability" (TRI), a reaction time quite important for practical PA systems which we call "reactivity".

Reactivity can be considered in various contexts, and in this paper, we choose to quantify TRI in term of the howling times in two distinct relevant scenarios commonly found in the scientific literature on AFR [8, 18] that can be extended to the general evaluation of AH systems :

- During initial convergence (TRII) which assesses how quickly the system can adapt and suppress feedback when it first appears.
- During change of acoustic paths (TRIC) which assesses how fast the system adapts to changing acoustic conditions, such as when the microphone or speakers are repositioned.

4 Proposed method for AH evaluation

This study thus delves into the realm of AH evaluation for PA system, aiming to provide a comprehensive methodology for assessing AH devices used in the context of real-world PA systems.

4.1 Measurement environment

While the various AH devices under test (DUT) may be hardware or software, a simulated environment was chosen for their measurement. Indeed, such a cost-effective environment may be varied easily, still offering accurate control and reproducibility. Moreover, it allows consistent results to be shared between many partners.

4.1.1 Principle

The measurement setup includes the AH system ($[H]$ block of Figure 1) as a VST plug-in (for software AH systems) or as a soundcard allowing to connect an external hardware device (for hardware AH systems). A PC is used to run all other parts of the measurement environment.

This environment is depicted by Figure 2. It features a signal source (an audio player here) which represents the talker. This signal is added to the output of a convolver plug-in allowing to simulate the Impulse Response (IR) of the electroacoustic path ($[F]$ block of figure 1). This IR may be switched when assessing the TRIC criterion (see section 3.2.3). The $[G]$ block of figure 1 is a pure linear gain which is the product of an analog hardware gain K_A and a digital gain K_D .

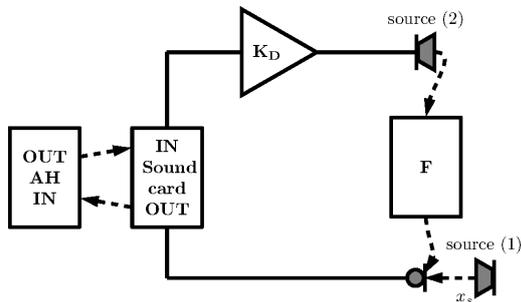


Fig. 2: Electroacoustic chain simulation diagram.

4.2 Software implementation

A VST host is used to connect all parts of the setup. We chose the open source software "Pedalboard 2" (based on the JUCE code for VST hosts) as it includes essential built-in plugins like an audio player, recorder, variable gain controls, VU meters, and channel selectors. Moreover it offers an OSC interface for seamless communication with Python, facilitating the execution of programmable action sequences.

A basic acoustic feedback simulation of Figure 2 is depicted in Figure 3 using Pedalboard 2. Gain levels, feedback, acoustic path switches and recording can be monitored via OSC commands. VU meters are employed to monitor audio levels, aiding in identifying the onset of howling even at low volumes. This implementation enables silent operation or connection to an additional speaker, facilitating operator monitoring of simulation performance.

The electroacoustic path is simulated using the convolver VST plugin 'R1 Convolution Rev' which user interface (UI) is shown in Figure 4, with the parameters corresponding to the IR used for TRIC test (an acoustic hall).

Simulations were conducted on a portable PC (Intel i7-1255U processor / 16 GB RAM). Although the CPU usage consistently remained below 20 %, occasional audio crackling was detected when using a block size below 128. To ensure smooth operation, a block size of 256 was employed, providing a safety margin against audio disruptions. This results into a consequent 38 ms latency. Latency's influence on the results will be addressed in the future. Preliminary investigations in the same configuration as used in this paper indicate that overall, the results' meaning remains unaffected

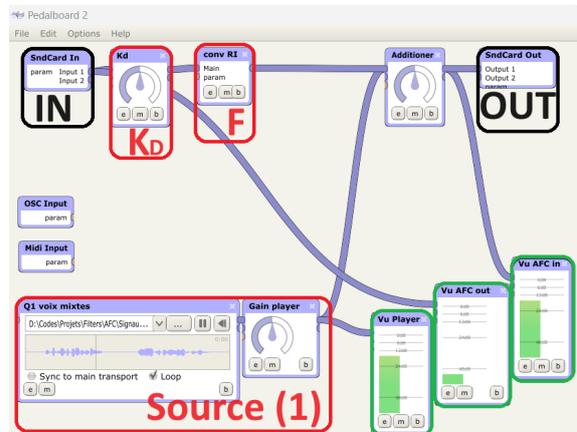


Fig. 3: Minimal setup for simulating acoustic feedback. In red, the player and acoustic feedback F , in green, VU meters, and in black, the sound card's input and output.



Fig. 4: Plugin 'R1 Convolution Reverb'. The IR selected is the Hall, with a RT 60 = 1.5s.

During the evaluation of the AH systems, they were connected to a Focusrite 4i4 sound card.

4.3 Evaluation protocol: recording

The whole evaluation actually consist first in a recording session and then in a post-processing part where the metrics are computed. The AH evaluation recording part includes the following steps, following initial configuration and source level adjustment:

1. Keeping $K_D = 0$, the operator tunes the sound-card input gain K_A with AH bypassed, trying to adjust the gain as close as possible to the howling threshold.

2. Freezing K_A , several gains K_D are then selected, increasing from -7 dB until the value for which howling can't be prevented (ASG). For each gain:

- Quality signals are recorded (for PESQ, see §3.2.2). The quality signal test is recorded once the AH system is stabilised (howling free).
- If the gain K_D is higher than zero, the TRII and TRIC signals are recorded (see §3.2.3). The TRII test signal is recorded immediately after resetting and unbypassing the AH system, while TRIC test signal is recorded immediately after switching the IR1 to the IR2.

Note that The input signals used for the PESQ test consist in two 8-second ITU speech signals: two sentences spoken by a female speaker and two spoken by a male speaker. The input signals used for the reactivity and the characterisation are white Gaussian noise of respectively, 25 and 10 seconds.

The switched second acoustic path IR2 corresponds to the modified hall depicted in Figure 4, while the main IR1 selected is the original version (obtained by resetting the parameters in the UI).

4.4 Evaluation protocol: post-processing

The metrics are introduced in a general manner in §3.2, while this section elaborates on the specific procedures we used to process them. While PESQ can be straightforwardly estimated using the ITU public code, there are multiple definitions available in the literature for ASG and reactivity.

For the gain, as stated above, the operator establishes a coarse 0 dB reference for the ASG (setting K_A factor). This is however not reliable enough to allow comparisons, especially between different operators. A first gain correction K_c is therefore performed, based on the IR measurement of the acoustic path ($[F]$ block). This is adapted from [8], considering that F and $H_{bypassed}$ are linear, stationary and evaluated. The correction K_c for the 0 reference of ASG is thus given by:

$$K_c[dB] = -20 \log_{10} \left[\max_{\omega \in P} |H_{bypassed}(\omega)F(\omega)| \right], \quad (1)$$

with $H_{bypassed}$ standing for the HR system bypassed with $K_D = 0$ dB and K_a set before the howling in order

to include latent phase shift and gain from the AH system. $P = \{\omega | \angle H_{bypassed}(\omega)F(\omega) = n2\pi\}$.

A second gain correction K_f is performed because the actual gain changes may not be only the ones tuned by the operator (K_D factor): the AH system itself may affect the gain. The actual gain is thus estimated from the spectra, using the following procedure. Considering x_{ref} a reference signal and x_{test} the signal for another gain K_f , the following minimization is performed to estimate K_f :

$$\min \left\| \|To(PSD(x_{ref}))\|K_f - \|To(PSD(x_{test}))\| \right\|^2 \quad (2)$$

Here, To represents the signal's FFT averaged in one-third octave bands and $PSD(x)$ is the power spectral density of x . The minimization is conducted within the frequency bands of 100 to 16000 Hz.

The actual gain K_{act} used as abscissa in the following figures is thus $K_{act} = K_f + K_c$.

When estimating the "Reactivity", both TRI delays are calculated between a change time and the onset of howling. In this paper, this howling onset is detected by comparing the error between a reference signal and a feedback signal ($\|x_{ref} - x_{test}\|/\|x_{ref}\|$), determining the upper error envelope, defining a threshold (e.g., 10 dB above max error when there is no howling), and estimating the time at which this threshold is exceeded. This requires that the recorded signals are long enough to include this transition.

5 First results

The evaluated products include four commercial products and two prototypes. The NHS products are the most usual solution in commercial systems whereas only a few AFR products are commercially available yet. Table 1 provides an overview of the broad properties of the tested products: half of them use NHS and the other half use AFR.

5.1 Sound quality versus gain increase

The results in Figure 5 illustrate the mean PESQ scores in relation to the gain increase K_{act} for all the products plus a reference pass-through configuration, considered as a reference. The ASG of each product is determined by the maximum gain reached by its curve. As stated

Product	Feature	Type
P1	NHS	Physical
P2	NHS	Physical
P3	AFR	Physical
P4	NHS	Plugin
P5	AFR	Physical
P6	AFR	Physical

Table 1: Table of measured AH products

above, 0 dB gain corresponds by definition to the maximum gain achievable without causing howling when no AH system is present. The pass-through has therefore an ASG of 0 dB. Starting the gain scale at -7 dB provides valuable insights into how the AH systems impact the sound quality in addition to the MSG change.

It can be seen that all scores fall below 3, indicating poor speech quality according to the PESQ scale, even in the case of the pass-through. This reflects the deviation from the original audio caused by the electroacoustic path (mainly reverberation). This has already been pointed out by previous studies which have shown that despite the lower scores due to added reverberation, standard quality evaluation methods can still maintain the meaningfulness of the evaluation, preserving the overall trends and tendencies. [31, 32, 33]. The scores given by Figure 5 should therefore be analyzed as relative values, taking the pass-through curve as a reference.

Keeping this in mind, results in Figure 5 exhibit two groups related to the AH method they employ. NHS products (P1, P2 and P4) tend to exhibit overall lower ASG (≈ 4 dB) than AFR products (P3, P5, P6) which reach ASG values above 15 dB). This is consistent with previous publications [8]. Moreover, all AFR-based products also improve the PESQ score by reducing reverberation, while NHS-based products do not change the sound quality for negative gains and tend to even degrade it for positive gains.

5.2 Reactivity versus gain increase

The results in Figure 6 show the reactivity results for the algorithms during initial convergence (TRII), while Figure 7 displays the results in the case of an acoustic path change (TRIC). Note that the abscissa gain values of Fig. 7 corresponds to the initial acoustic path which allows a higher MSG than the modified one. This

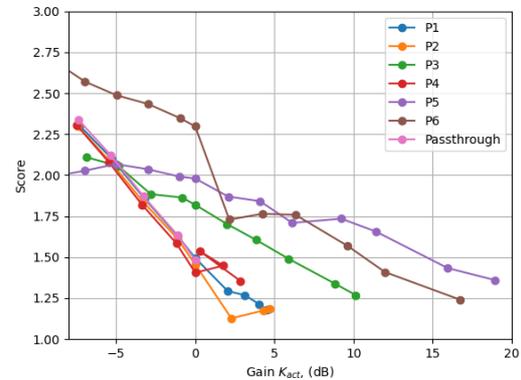


Fig. 5: Mean PESQ quality scores obtained using different AH versus gain increase.

explains why howling may occur even for 0 dB in this figure.

For the NHS products, Figure 6 illustrates a relatively fast convergence (below 2 seconds) only for added gain lower than 2 dB, whereas the AFR products converge even for gains of at least 8 dB. Notably, P3 demonstrates instant convergence up to 10 dB. The results in Figure 7 demonstrate a similar overall trend albeit less pronounced. NHS products do not seem robust to quick changes of the electroacoustic path, P1 being the fastest one but still needing about 10 s with a gain of 2 dB. Globally, AFR products seem more robust but show distinct TRI performances, P3 being the fastest.

In relation with Figure 5, this highlights a clear trade-off between convergence times and PESQ quality scores. Slower convergence seems to preserve speech quality more effectively.

6 Conclusion

The aim of this work was to bridge a gap by proposing a protocol allowing to compare all AH principles between them, in the context of PA systems, and dealing with commercial products as well as laboratory moc-up. Moreover, we wanted to allow comparison of evaluation results performed by various operators or teams.

The protocol described above is a first step in this direction; it could compare very different systems (NHS- or AFR- based) and highlight coarse tendencies but

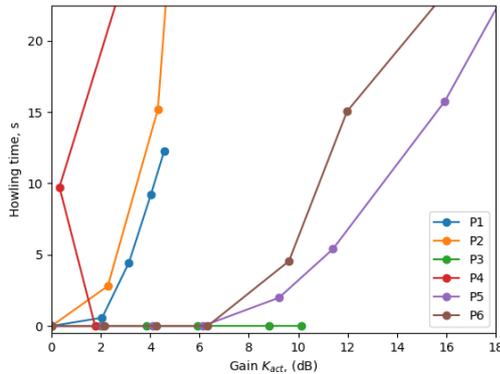


Fig. 6: Howling times during AH convergence versus gain increase.

also smaller differences resulting from different design trade-off. The main tendencies are consistent with previous publications, clearly showing the differences between AH principles.

The proposed protocol is implemented using a standard PC and a widespread soundcard, using open-source and cheap software: it should thus be quite easy to duplicate by other teams if needed. We hope it would thus provide valuable insights for decision-making when choosing an AFC system based on specific requirements and priorities, but also for designing or tuning new products or including AH technology for new applications.

While the current evaluation method already allows to distinguish between different products in terms of a few accepted criteria, it can obviously be improved in some respects - hopefully through interactions with other interested teams.

The proposed implementation allows to vary easily the IR's used to emulate the electroacoustic path, which should be representative of a targeted application (broadly ranging from teleconference rooms to houses of wisdom). A suitable selection of IR's should be defined, and the corresponding results compared. The TRIC test (time to adapt to a change of electroacoustic path) may also be more representative by using more realistic changes than switching between quite different IR's.

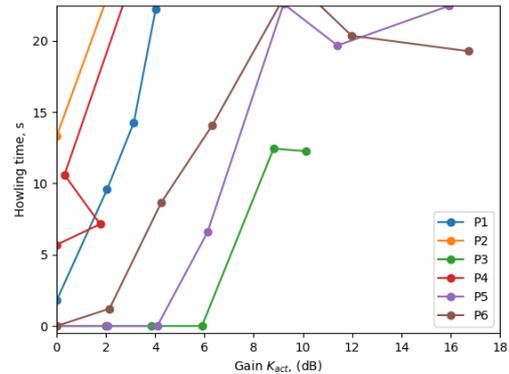


Fig. 7: Howling times during AH convergence after switching the acoustic path versus gain increase.

The influence of the implementation details (simulation and convolution latency, signals SNR) should be investigated and specified in order to keep results comparable between different setup.

The quality evaluation, based only on the PESQ score, does not reflect the listener experience for musical diffusion. A complementary score could be defined, although this might lead to significant licence costs.

All these aspects are the object of current work, including the comparison of additional existing products and AH principles. Given the substantial resources required for these endeavors, we welcome any cooperation and collaboration to further enhance our efforts in this field.

References

- [1] T-REC-G.131, *Talker echo and its control*, ITU, Geneva (CH), 2003.
- [2] Agnew, J., "Acoustic Feedback and Other Audible Artifacts in Hearing Aids," *Trends in Amplification*, 1(2), pp. 45–82, 1996.
- [3] Boner, C. and Boner, C., "Behavior of Sound System Response Immediately Below Feedback," *J. Audio Eng. Soc.*, 14(3), pp. 200–203, 1966.
- [4] Davis, G. and Jones, R., *The sound reinforcement handbook 2nd ed.*, Hal Leonard, Milwaukee (US), 1990.

- [5] Schroeder, M. and Kuttruff, K., "On Frequency Response Curves in Rooms. Comparison of Experimental, Theoretical, and Monte Carlo Results for the Average Frequency Spacing between Maxima," *J. Acoust. Soc. Am.*, 34(1), pp. 76–80, 1962.
- [6] Poletti, M., "The Stability of Single and Multichannel Sound Systems," *Acta Acustica / Acustica*, 86(1), pp. 163–178, 2000.
- [7] Von Wangenheim, L., "On the Barkhausen and Nyquist stability criteria," *Analog Integr. Circ. Sig. Proc.*, 66(1), pp. 139–141, 2011.
- [8] van Waterschoot, T. and Moonen, M., "Fifty Years of Acoustic Feedback Control: State of the Art and Future Challenges," *Proceedings of the IEEE*, 99(2), pp. 288–327, 2011.
- [9] Thuillier, E., Lähdeoja, O., and Välimäki, V., "Feedback Control in an Actuated Acoustic Guitar using Frequency Shifting," *J. Audio Eng. Soc.*, 67(6), p. 373–381, 2019.
- [10] Nielsen, J. and Svensson, U., "Performance of some linear time-varying systems in control of acoustic feedback," *J. Acoust. Soc. Am.*, 106(1), p. 240–254, 1999.
- [11] Guo, M., Jensen, S., Jensen, J., and Grant, S., "On the Use of a Phase Modulation Method for Decorrelation in Acoustic Feedback Cancellation," in *Proc. EUSIPCO*, Bucharest (RO), 2012.
- [12] Patronis, J., "Electronic Detection of Acoustic Feedback and Automatic Sound System Gain Control," *J. Audio Eng. Soc.*, 26(5), pp. 323–326, 1978.
- [13] Osmanovic, N., Clarke, V., and Velandia, E., "An In-Flight Low Latency Acoustic Feedback Cancellation Algorithm," in *Proc. 123rd Audio Eng. Soc. Conv.*, New York (US), 2007.
- [14] Kuo, S. and Chen, J., "New adaptive IIR notch filter and its application to howling control in speakerphone system," *Electronics Letters*, 28(8), pp. 764–766, 1992.
- [15] Bispo, B. and Freitas, D., "On the use of cepstral analysis in acoustic feedback cancellation," *Dig. Sig. Proc.*, 44, p. 88–101, 2015.
- [16] Bernardi, G., Van Waterschoot, T., Wouters, J., and Moonen, M., "Adaptive Feedback Cancellation Using a Partitioned-Block Frequency-Domain Kalman Filter Approach With PEM-Based Signal Prewhitening," *IEEE/ACM Trans. Audio, Speech, Lang. Proc.*, 25(9), p. 1784–1798, 2017.
- [17] Yang, F. and Yang, J., "Optimal Step-Size Control of the Partitioned Block Frequency-Domain Adaptive Filter," *IEEE Trans. Circ. Systems II*, 65(6), p. 814–818, 2018.
- [18] Tran, L. and Nordholm, S., "A Switched Algorithm for Adaptive Feedback Cancellation Using Pre-Filters in Hearing Aids," *Audiology Research*, 11(3), p. 389–409, 2021.
- [19] Connor, W., "Experimental Investigation of Sound-System-Room Feedback," *J. Audio Eng. Soc.*, 21(1), pp. 27–32, 1973.
- [20] T-REC-G.167, *Acoustic echo controllers*, ITU, Geneva (CH), 1993.
- [21] Bispo, B. and Freitas, D., "Performance Evaluation of Acoustic Feedback Cancellation Methods in Single-Microphone and Multiple-Loudspeakers Public Address Systems," in M. Obaidat, A. Holzinger, and J. Filipe, editors, *E-Business and Telecommunications*, pp. 473–495, Springer, 2015.
- [22] Guo, M., Jensen, S., and Jensen, J., "Evaluation of State-of-the-Art Acoustic Feedback Cancellation Systems for Hearing Aids," *J. Audio Eng. Soc.*, 61(3), p. 125–137, 2013.
- [23] van Waterschoot, T. and Moonen, M., "Assessing the Acoustic Feedback Control Performance of Adaptive Feedback Cancellation in Sound Reinforcement Systems," in *2009 17th European Signal Processing Conference*, pp. 1997–2001, 2009.
- [24] Shin, M., Wang, S., Bentler, R., and He, S., "New feedback detection method for performance evaluation of hearing aids," *J. Sound Vib.*, 302(1-2), p. 350–360, 2007.
- [25] Waterschoot, T. v. and Moonen, M., "Comparative Evaluation of Howling Detection Criteria in Notch-Filter-Based Howling Suppression," *J. Audio Eng. Soc.*, 58(11), p. 923–940, 2010.

- [26] Peng, R., Li, J., Zheng, C., Chen, X., and Li, X., “Cepstrum-Based Preprocessing for Howling Detection in Speech Applications,” in Proc. 135th Audio Eng. Soc. Conv., Paper 8978, 2013.
- [27] Faccenda, F., Squartini, S., Principi, E., Gabrielli, L., and Piazza, F., “An Embedded-Processor Driven Test Bench for Acoustic Feedback Cancellation in Real Environments,” in Proc. 134th Audio Eng. Soc. Conv., Paper 8835, 2018.
- [28] Spriet, A., Moonen, M., and Wouters, J., “Evaluation of feedback reduction techniques in hearing aids based on physical performance measures,” J. Acoust. Soc. Am., 128(3), pp. 1245–1261, 2010.
- [29] Torcoli, M., Kastner, T., and Herre, J., “Objective Measures of Perceptual Audio Quality Reviewed: An Evaluation of Their Application Domain Dependence,” IEEE/ACM Trans. Audio, Speech, Language Process., 29, pp. 1530–1541, 2021.
- [30] Schepker, H., Nordholm, S., and Doclo, S., “Acoustic Feedback Suppression for Multi-Microphone Hearing Devices Using a Soft-Constrained Null-Steering Beamformer,” IEEE/ACM Trans. Audio, Speech, Language Process., 28, pp. 929–940, 2020.
- [31] et Al., d., “Reverberation assessment in audioband speech signals for telepresence systems,” in Proceedings of the Int. Conf. Signal Proc. and Mult. App., pp. 257–262, SciTePress - Science and Technology Publications, Porto, Portugal, 2008.
- [32] et Al., d., “Quality Evaluation of Reverberation in Audioband Speech Signals,” in e-Business and Telecommunications, Commun. Comput. Inf. Sci., pp. 384–396, Springer, Berlin, Heidelberg, 2009.
- [33] Naylor, P. A., Gaubitch, N. D., et al., Speech dereverberation, volume 2, Springer, 2010.